



Prüf- und Zertifizierungsstelle

ZELM Ex



(1) **EC-TYPE-EXAMINATION CERTIFICATE**  
(Translation)

(2) Equipment and Protective Systems Intended for Use in Potentially Explosive Atmospheres - **Directive 94/9/EC**

(3) EC-TYPE-EXAMINATION CERTIFICATE Number:

**ZELM 99 ATEX 0008 X**

(4) Equipment: **Density Meter DIMF \*.\* T\*\* ...**

(5) Manufacturer: **Bopp & Reuther Messtechnik GmbH**

(6) Address: **D-68305 Mannheim**

(7) This equipment and any acceptable variation thereto are specified in the schedule to this certificate and the documents therein referred to.

(8) The Prüf- und Zertifizierungsstelle ZELM Ex, notified body No. 0820 in accordance with Article 9 of the Council Directive 94/9/EC of 23 March 1994, certifies that this equipment has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of equipment and protective systems intended for use in potentially explosive atmospheres, given in Annex II to the Directive.

The examination and test results are recorded in the confidential report ZELM Ex 0569815009.

(9) Compliance with the Essential Health and Safety Requirements has been assured by compliance with:

**EN 50 014: 1997**

**EN 50 020: 1994**

**EN 50 284: 1997**

(10) If the sign "X" is placed after the certificate number, it indicates that the equipment is subject to special conditions for safe use specified in the schedule to this certificate.

(11) This EC-type-examination Certificate relates only to the design and construction of the specified equipment in accordance with Directive 94/9/EC. Further requirements of this Directive apply to the manufacture and supply of this equipment.


(12) The marking of the equipment shall include the following:



**II 1/2 G EEx ia IIC T4**

Zertifizierungsstelle **ZELM Ex**

  
Dipl.-Ing. Harald Zelm

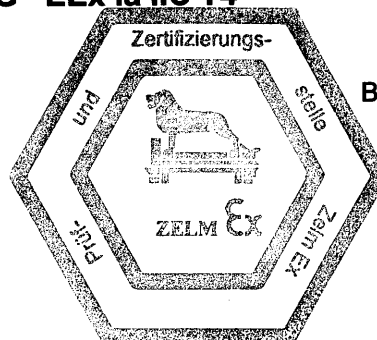

Braunschweig, October 29, 1999

Sheet 1/3

EC-type-examination Certificates without signature and stamp shall not be valid. The certificates may be circulated only without alteration. Extracts or alterations are subject to approval by the Prüf- und Zertifizierungsstelle ZELM Ex. In case of dispute, the German text shall prevail.



(13)

## SCHEDULE

(14)

### EC-TYPE-EXAMINATION CERTIFICATE ZELM 99 ATEX 0008 X

(15) Description of equipment

The density meter is made for continuous measuring of density or concentration of liquids, liquid mixtures or multi-phase fluids.

Essentially it consists of the fork enclosure, made of stainless steel containing the pipe fork or the vibration fork with the measured fluid inside, and the electronical transmitter within a housing of cast aluminium alloy. Variation of the natural frequency of the fork due to density variation of the fluid is measured by the sensor coil and transformed by the transmitter into a density-proportional signal. The transmitter housing is mounted on the fork enclosure with an extension tube or separated as wall mounting. In this case there is a terminal box mounted on the extension tube.

The model DIMF \*. \* T\*\* ... density meter is intended for use in potentially explosive atmospheres. Its supply circuit must be a certified intrinsically safe supply and signal circuit

The density meter permits bidirectional communication by HART protocol.

Dependent on the measured fluid the fork may be assessed as category 1G. Also a flammable non-explosive medium is possible.

#### Electrical data

supply- / signal circuit  
(KL 1.1 and KL1.2)

type of protection Intrinsic Safety EEx ia IIC

only for connection to certified intrinsically safe circuits with the following max. values:

$$U_o = 30 \text{ V}$$

$$I_o = 110 \text{ mA}$$

$$P_o = 825 \text{ mW}$$

effective internal capacitance and inductance:

$$C_i \leq 34 \text{ nF}$$

$$L_i \leq 0,6 \text{ mH}$$

(16) Report No. ZELM Ex 0569815009

(17) Special conditions for safe use

The equipment is fit for an ambient temperature of  $-40 \text{ }^{\circ}\text{C}$  up to  $+58 \text{ }^{\circ}\text{C}$  related to transmitter electronics. Temperature of the measured fluid may come up to  $+210 \text{ }^{\circ}\text{C}$ .

The assignment of temperature class and maximum medium and ambient temperature is shown as follows:



Optional heat insulation may cover the half of the extension tube.  
Ambient temperature has to be met just beyond the electronics or terminal housing.  
Minimum medium and ambient temperature is  $-40\text{ }^{\circ}\text{C}$ .

DIMF *.* TV* (Extension tube)			
Class	T ambient [ $^{\circ}\text{C}$ ] electronics	T medium [ $^{\circ}\text{C}$ ]	Type
T2	46	210	<b>H</b>
T3	46	200	High temperature
T3	49	170	
T3	50	150	<b>S+H</b>
T4	52	135	Standard temperature
T4	54	110	and
T4	58	60	High temperature

DIMF *.* TW* (Wall mounting)			
Electronics Ambient temp.:		58 $^{\circ}\text{C}$	
Class	T ambient [ $^{\circ}\text{C}$ ] terminal box	T medium [ $^{\circ}\text{C}$ ]	Type
T2	67	210	<b>H</b>
T3	68	200	High temperature
T3	71	170	
T3	73	150	<b>S+H</b>
T4	74	135	Standard temperature
T4	77	110	and
T4	80	80	High temperature


Due to these limits the maximum temperature of electronic parts will meet the amount of  $60\text{ }^{\circ}\text{C}$ .


(18) Essential Health and Safety Requirements

met by standards

Zertifizierungsstelle ZELM Ex

Braunschweig, October 29, 1999

  
Dipl.-Ing. Harald Zelm

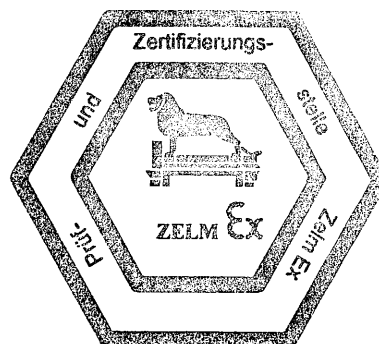



Prüf- und Zertifizierungsstelle

ZELM Ex



## 1. Supplement

(Supplement according to EC-Directive 94/9 Annex III letter 6)

to EC-type-examination Certificate

**ZELM 99 ATEX 0008 X**

Equipment: **Density Meter DIMF \*.\* T\*\*...**  
Manufacturer: **Bopp & Reuther Messtechnik GmbH**  
Address: **D-68305 Mannheim**

### Description of supplement

The address is changed to: **D-67346 Speyer**

The Density Meter DIMF \*.\* T\*\*... will be supplemented by an alternative version with an increased pipe diameter. The type designation of this new version is DIMF 2.1 T\*\*....

The modifications concern to the construction and the type designation of the equipment.

The "Special conditions for safe use" are supplemented.

All further data remain unchanged and are valid also for this 1. Supplement.

### Report No.

ZELM Ex 1160415273

### Special conditions for safe use

The special conditions of the EC-type-examination Certificate ZELM 99 ATEX 0008 X are valid further on. The following is additionally applied:

For the operation with mediums which require the category 1, impact and friction - for instance by solid parts in the medium - must be safely avoided.

### Essential Health and Safety Requirements

The Essential Health and Safety Requirements are further met by adherence to the standards which are given in the EC-type-examination Certificate.

Zertifizierungsstelle ZELM Ex



Braunschweig, October 18, 2004

Adolf Gruber

Sheet 1 / 1

## 2. Supplement

(Supplement according to EC-Directive 94/9 Annex III letter 6)

**ZELM ex**

to EC-type-examination Certificate

### ZELM 99 ATEX 0008 X

Equipment: **Density Meter DIMF \*.\* T\*\*...**  
Manufacturer: **Bopp & Reuther Messtechnik GmbH**  
Address: **D-67346 Speyer**

#### Description of supplement

The conformity of the equipment with the actual standards was reviewed within the scope of the 2. Supplement. The marking was aligned accordingly. There were no additional changes made on the equipment.

The marking in the future is:



**II 1/2 G Ex ia IIC T4**

All further data as well as the special conditions for safe use according the EC-type examination certificate and the 1. Supplement are not changed, and are also valid for this 2. Supplement. The equipment is allowed to be manufactured in the future also in accordance to this first supplement.

#### Report No.

ZELM Ex 1621015810

#### Essential Health and Safety Requirements

The conformity of the equipment with the actual standards was reviewed within the scope of the 2. Supplement. The essential health and safety requirements are still fulfilled by compliance with the following Standards:

**EN 60079-0:2009**

**EN 60079-11:2007**

**EN 60079-26:2006**

Braunschweig, October 15, 2010

**ZELM ex**

**Zertifizierungs-  
stelle**

**Zertifizierungsstelle ZELM ex  
Dipl.-Ing. Harald Zelm**

**ZELM  
ex**

Sheet 1 of 1

EC-type-examination Certificates without signature and stamp are not valid. This EC-type-examination Certificate may only be circulated without alteration. Extracts or alterations are subject to approval by the Prüf- und Zertifizierungsstelle ZELM ex. This English version is based on the German text. In the case of dispute, the German text shall prevail.

**ZELM ex**  
Prüf- und Zertifizierungsstelle  
Siekgraben 56 · D-38124 Braunschweig

# 3. Supplement



(Supplement according to EC-Directive 94/9 Annex III letter 6)

## to EC-type-examination Certificate

### ZELM 99 ATEX 0008 X

Equipment: **Density Meter DIMF \*.\* T\*\*...**  
 Manufacturer: **Bopp & Reuther Messtechnik GmbH**  
 Address: **D-67346 Speyer**

#### Description of supplement

The conformity of the equipment with the actual standards was reviewed within the scope of the 3. Supplement. The marking was aligned at manufacturers request according to EN 60079-0:2012 + A11:2013, section 29.4. There were no additional changes made on the equipment.

The marking in the future is:



**II 1/2 G Ex ia IIC T4 Ga/Gb**

All further data as well as the special conditions for safe use according the EC-type examination certificate including the 1. and 2. Supplement are not changed, and are also valid for this 3. Supplement. The equipment shall only be manufactured in the future in accordance to this third supplement.

#### Report No.

ZELM Ex 13815191142

#### Essential Health and Safety Requirements

The conformity of the equipment with the actual standards was reviewed within the scope of the 3. Supplement.

The essential health and safety requirements are still fulfilled by compliance with the following Standards:

**EN 60079-0:2012 + A11:2013    EN 60079-11:2012    EN 60079-26:2015**

Braunschweig, 2015-12-18



**Zertifizierungs-  
stelle**

Zertifizierungsstelle ZELM ex  
Dipl.-Ing. Harald Zelm



Sheet 1 of 1

EC-type-examination Certificates without signature and stamp are not valid. This EC-type-examination Certificate may only be circulated without alteration. Extracts or alterations are subject to approval by the Prüf- und Zertifizierungsstelle ZELM ex. This English version is based on the German text. In the case of dispute, the German text shall prevail.

ZELM ex  
Prüf- und Zertifizierungsstelle  
Siekgraben 56 · D-38124 Braunschweig